

User Manual

LC100-A Digital L/C Meter

Inductance Capacitance Meter

Rev. 4.1
2010.9.22

Features:

Based on the L/C resonance principle

High speed microcontroller's precision computation

Measuring range below 1uH and 1pF

Especially qualify in microwave manufacture and measuring switching power supply transformer, filter inductance and so on.

The LC100 series divided into the LC100-S ground form and the LC100-A entire function two models, LC100-A has four measuring range position:

1. C rangeCapacitance (0.01pF-10uF)
2. L rangeInductance (0.001uH-100mH)
3. HL rangeBig inductance (0.001mH-100H)
4. HC rangeBig capacitance range (1uF-100mF)


All files position are automatic measuring ranges, it is easy to operate. Specification is as follows:

1. Technique data:

	Item	Parameter
Capacitance Accuracy	0.01pF-1pF	5%
	1pF-1uF	1%
	1uF-10uF	5%
Min Capacitance Resolution (C Files)		0.01pF
Inductance Accuracy	0.001uH-1uH	5%
	1uH-100mH	1%
Min Inductance Resolution (L Files)		0.001uH

Big Inductance Accuracy	100mH-1H	1%
	1H-100H	5%
Min Resolution of Big Inductance (HL Files)		0.001mH
Big Capacitance Accuracy	1uF-100mF	5%
Min Resolution of Big Capacitance (HC Files)		0.01uF
Frequency	L Files、C Files	Abt. 500kHz
	HL Files	Abt. 500Hz
Measuring mode		LC Resonance
Display mode		1602 LCD
Display digit		4
Interface		Mini USB & 5.5DC Socket
Supply Voltage		5V

2. Picture

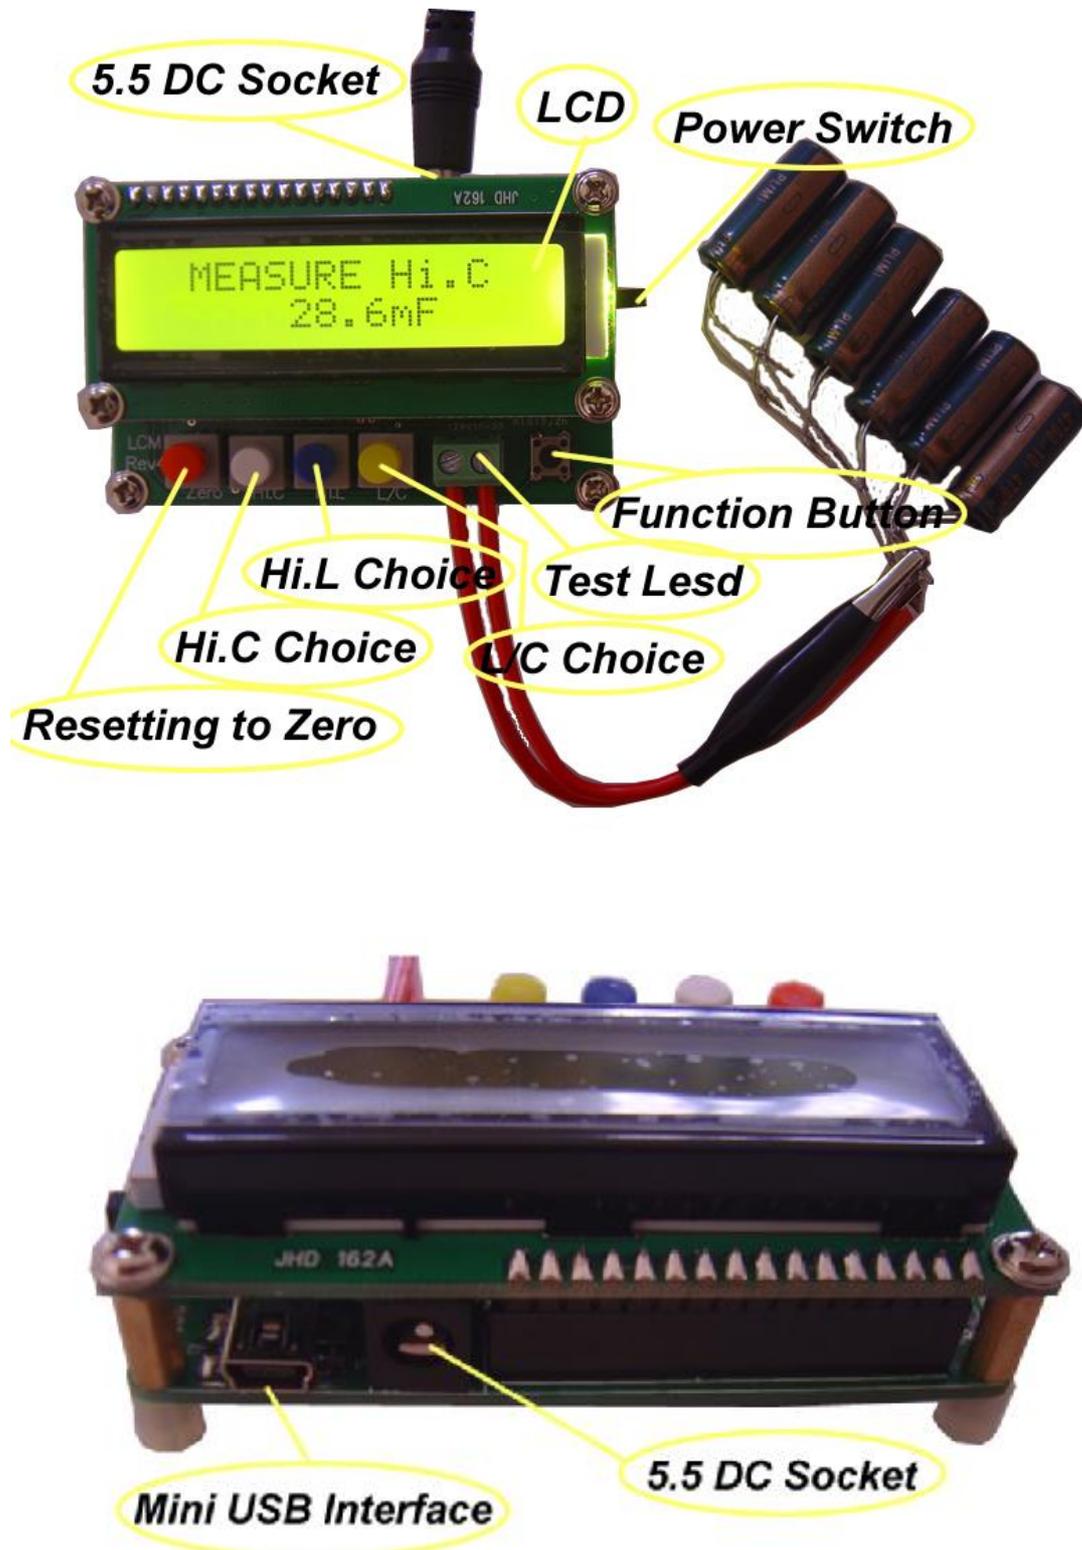

Function of five buttons:

Red: Reset

Write: Big Capacitance HiC Choice (With self-locking)

Blue: Big Inductance HiL Choice (with self-locking)

Yellow: L/C(with self-locking)

Black: Function button

Details as follows (Press “1”, Release “0”, “X” random)

LC100-A Function table

Hi.C	Hi.L	L/C	Corresponding function
0	0	0	Small Capacitance(C)
0	0	1	Small Inductance(L)
0	1	1	Big Inductance (HL)
0	1	0	Error, please modify
0	X	X	Big Capacitance (HC)

Interface: Mini USB & 5.5DC Socket (inner: positive pole, outer: negative pole)

3. Direction for use

- (1). Switch on the L/C Meter
- (2). Chose the corresponding files, inductance: Lx, capacitance: Cx, big inductance: HL, big capacitance: HC. Display as follows (testing terminal open loop) :

Inductance: MEASURE Lx

OVER RANGE

Capacitance: MEASURE Cx	0.00pF
Big inductance: MEASURE Hi.L	OVER RANGE
Big capacitance: MEASURE Hi.C	0.00pF
Display as follows(testing terminal short circuit):	
Big inductance: MEASURE Hi.L	0.000mH
Inductance: MEASURE Lx	0.000uH
Capacitance: MEASURE Cx	OVER RANGE

(3).When testing terminal open loop the measured value of capacitance is not “0”, or witch of the inductance is not “0” as the testing terminal short circuit, you can reset to “0” by ways of capacitance model and inductance model, as follows:

(a) Capacitance model

Press red button as testing terminal open loop, it displays “CALCULATING...”, keep pressing for one second, when “CALCULATING...OK” displayed, resetting to “0” is finished, and “0.00pF” is displayed, then capacitances can be measured.

(b) Inductance model

Press red button as testing terminal shirt circuit, it displays “0.000uH” or “0.000mH”, and then inductances can be measured.

(4). Please press black function button as results displayed, and

corresponding frequency will be displayed.

4. Note:

1. Please reset to “0” before testing a capacitance or an inductance, or errors may be appeared. Even if “0” displayed before measuring, resetting to “0” is needed.
2. At the time of resetting to “0”, when “CALCULATING...OK” appeared, please keep pressing for 2 to 3 seconds, and the parameter written to “<DATA SAVED>” will be prompted, then release.
3. Resetting to “0” is forbidden as components are being measured. If you do it, please shut down immediately and restart, then reset to “0”.
4. The time of measuring a big capacitance (above 10mF) may be more than one second, and it needs seven to eight seconds to get the measured value of the capacitance (100mF).
5. Forbid to measure a capacitance which is not discharged, otherwise it may damage the mainframe.

5. Package content

1. LC100-A L/C Meter.....1
2. mini USB cable.....1